

# TEST REPORT

(Electronic version)



No:200109116

VERIFICATION WEBSITE: [www.gttc.net.cn](http://www.gttc.net.cn)

VERIFICATION CODE: QGIV-4816-54

ISSUE DATE:2020-05-07

二维码载报告



APPLICANT: GUANGZHOU SHUFANG MEDICAL INSTRUMENTS CO., LTD  
ADDRESS: ROOM 713, NO. 34, QIFU ROAD, YUNCHENG STREET, BAIYUN DISTRICT, GUANGZHOU, CHINA

INFORMATION CONFIRMED BY APPLICANT:

KN95 FACE MASK

QUANTITY: FORTY-FIVE PIECES

DATE RECEIVED/DATE TEST STARTED: 2020-05-07

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M


NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT  
"----" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200072746.  
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).  
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.  
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

WanLi Hu ENGINEER




PAGE 1 OF 4

# TEST REPORT

(Electronic version)

No:200109116

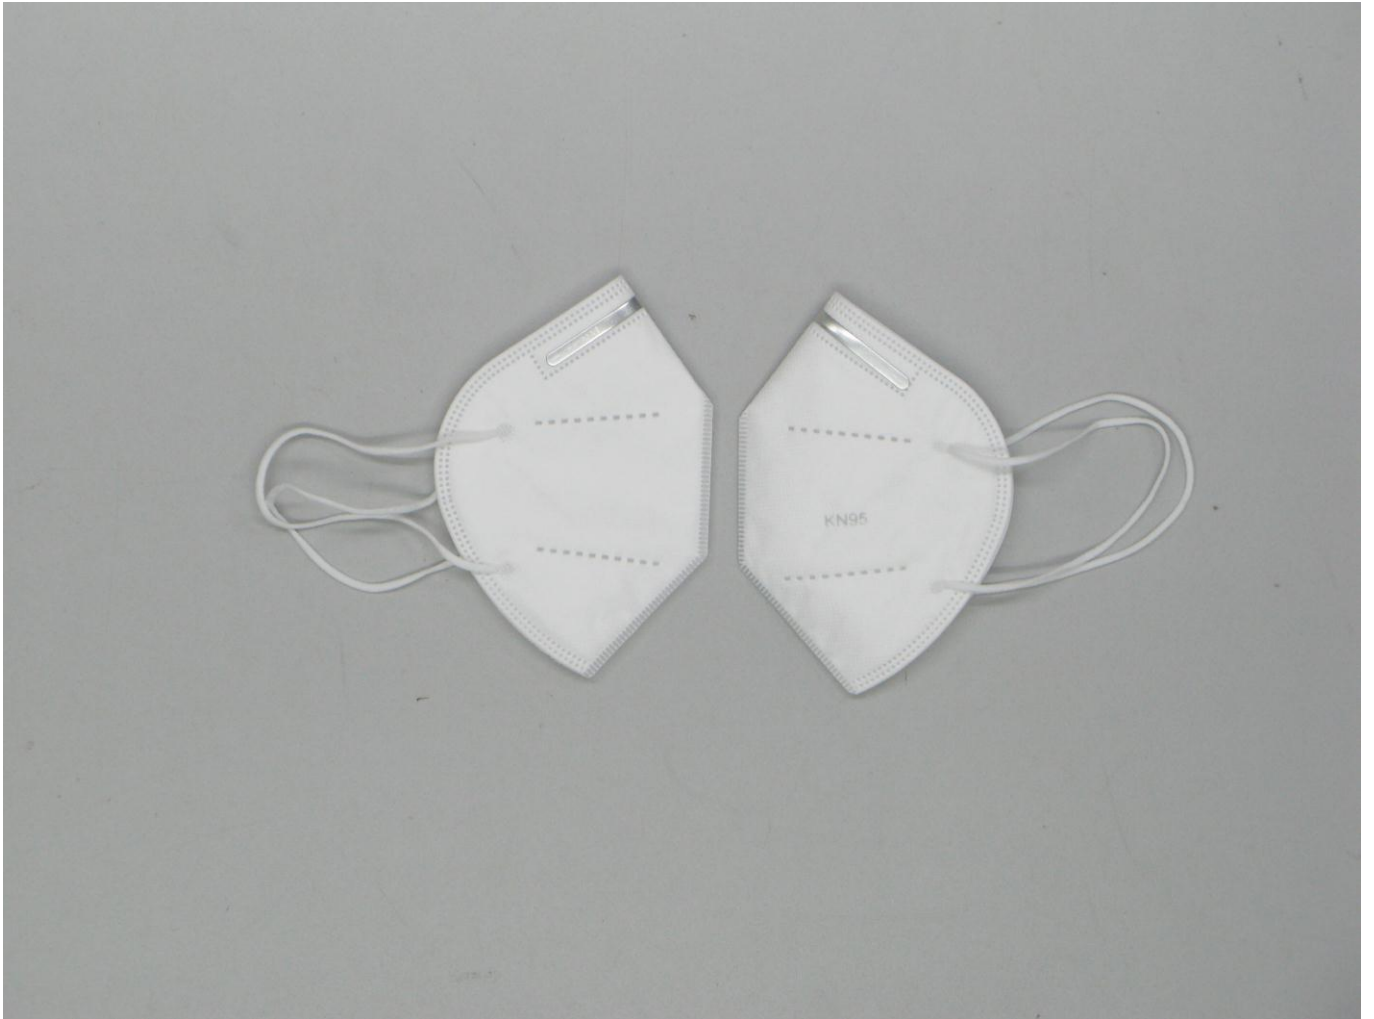

# TEST REPORT

(Electronic version)

No:200109116

## FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m<sup>3</sup>, TEMP:24.0℃, RH:36.4%)

### FILTRATION EFFICIENCY(%) :

#### UNTREATED SAMPLE

1# 99.242  
2# 99.311  
3# 99.356  
4# 99.180  
5# 99.275  
6# 99.142  
7# 98.96  
8# 99.097  
9# 99.410  
10# 99.354

#### CONDITIONING TREATED

1# 98.03  
2# 97.88  
3# 97.96  
4# 96.79  
5# 97.21

### REQUIREMENT

#### FILTRATION EFFICIENCY(%) :

≥95.0  
(KN95)  
(GB 2626-2006)

## INSPIRATORY RESISTANCE(Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

### UNTREATED SAMPLE:

1# 89.3  
2# 91.8

### PRETREATMENT SAMPLE:

1# 97.6  
2# 100.9

### REQUIREMENT

≤350  
(GB 2626-2006)

## EXPIRATORY RESISTANCE(Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

### UNTREATED SAMPLE:

1# 76.1  
2# 77.7

### PRETREATMENT SAMPLE:

1# 84.4  
2# 87.5

### REQUIREMENT

≤250  
(GB 2626-2006)

## FLAMMABILITY(s)

(GB 2626-2006 6.15)

### AFTERFLAME TIME

#### UNTREATED SAMPLE

1# 0.0  
2# 0.0

#### CONDITIONING TREATED

3# 0.0  
4# 0.0

### REQUIREMENT

AFTERFLAME TIME  
≤5  
(GB 2626-2006)



PAGE 3 OF 4

# TEST REPORT

(Electronic version)

No:200109116

---

## HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

## REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST

PARTS OF MASK SHOULD NOT SLIP OR BREAK

UNDER 10N TENSION FOR 10S.

(GB 2626-2006)

---



—End of Report—

PAGE 4 OF 4